

# VALERIA

## POWDER FREE BLUE NITRILE EXAMINATION GLOVES

# L

Büyük/Large

İki ele de uyumlu  
Ambidextrous

Tek kullanımlık  
Single use only

Steril değildir  
Non-Sterile

Cerrahi eldiven değildir.  
Ameliyatlarda kullanılamaz.  
This is not a surgical glove.  
Do not use in surgery.

# CE



## PUDRASIZ MAVİ NİTRİL MUAYENE ELĐİVENİ

İfınız / Push



Latex free  
Latex içermez

# **VALERIA**

***PUDRASIZ MAVI NITRİL MUAYENE ELDİVENİ***

AQL= 1.5

Steri edilmemiştir.  
Non-sterile  
EN 465-2




Product Service

# CERTIFICATE

No. Q1N 15 09 61155 010

**Holder of Certificate:** TERANG NUSA SDN. BHD.

1, Jalan 8, Pengkalan Chepa 2  
Industrial Zone  
16100 Kota Bharu, Kelantan  
MALAYSIA

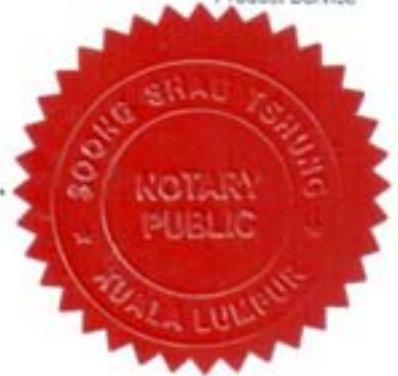

**Facility(ies):**

TERANG NUSA SDN. BHD.  
1, Jalan 8, Pengkalan Chepa 2, Industrial Zone,  
16100 Kota Bharu, Kelantan, MALAYSIA



**Certification Mark:**



**Scope of Certificate:** Design and Development, Production and Distribution of Sterilized Surgical and Examination Gloves, Non-Sterile Examination Gloves and Sterile Radiation Reducing Surgical Gloves

**Applied Standard(s):**

EN ISO 13485:2012 + AC:2012  
Medical devices - Quality management systems - Requirements for regulatory purposes (ISO 13485:2003 + Cor. 1:2009)  
DIN EN ISO 13485:2012

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). See also notes overleaf.

**Report No.:** MYQMH0615067-721413143

**Valid from:** 2015-11-18  
**Valid until:** 2018-10-31



This is to certify that the signature appears on this document/Certificate/ Marriage Certificate/Birth/Death Certificate is that of SOONG SHAU TSHUNG who is Notary Public on Date: 2015-11-15. The Ministry of Foreign Affairs, Malaysia is responsible for the accuracy of the information contained therein.



Mohd Ruslan Mohd Nor  
Consular Officer  
Consular Division  
Putrajaya Malaysia

DAkks  
Deutsche  
Akreditierungsstelle  
D-2M-11121-01-00



26 APR 2018

ZERTIFIKAT ◆ CERTIFICATE ◆ 認証証書 ◆ CERTIFICADO ◆ CERTIFICAT

TERANGNUSA (M) SDN BHD  
 PLO 9 & 18, KWSN PERINDUSTRIAN KLUANG  
 86007 KLUANG, JOHOR, MALAYSIA  
 TEL : 07-7879812

## Certificate of Analysis

Consignee : Issued date : 28/06/2019  
 Type of gloves : ENDBHF32 Invoice No. :  
 Exam. Nitrile, Powder Free Gloves Order No. :  
 Certificate No. : 001/15

Test Performed	Standard EN 455	Results
Inspection Plan ISO 2859		
Watertight test failures(1000ml) GI AQL 1.5	500 - 14 - 15	6
Dimension Length (mm) S2 AQL 4.0	>= 240	242 - 246
Width (mm)		
XS	NA	NA
S	NA	NA
M	95 ± 10	96
L	NA	NA
XL	NA	NA
Thickness (mm)		
Cuff	NA	0.05 - 0.06
Palm	NA	0.06 - 0.07
Finger	NA	0.09 - 0.10
Force at break throughout shelf life S2 AQL 4 C		
Force at break (median)	Min 5.0 N	5.972 N
Force at break after challenge testing S2 AQL 4 C		
Force at break (median)	Min 5.0 N	5.517 N


\* Force @ break after challenge testing carried out as per EN 455 part 2 at 70°C for 7 days.  
 \* The inspection plan is following according to ISO 2859 GI AQL 1.5 (Water tight test)  
 S2 AQL 4.0 (Others)

Protein content	Test Standard EN455-3	NA
Powder content	Max. 2.0 mg/glove	1.00 mg/glove

Note :

Lot No : NA  
 Manufacturing date : 2020-06  
 Expiry date : 2024-05

Head of testing section :

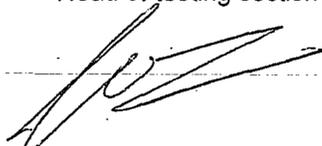

Vincent Chua Kim Chok  
 QA Manager

**UNCONTROLLED  
 DOCUMENT**  
 (For Reference Only)



TERANG NUSA Sdn Bhd

K041436

510(k) Submission for NUZONE X2 Surgical Glove Powderfree

AUG 20 2004

## 510(k) Summary

Submitter Name	Terang Nusa Sdn Bhd
Submitter Address	1, Jalan 8 Pengkalan Chepa 2 Industrial Zone 16100 Kota Bharu, Kelantan, Malaysia.
Submitter Telephone	+60 9 7747171
Submitter Fax	+60 9 7747757
Contact Person	LOW, Chin Guan
Date of preparation	09 May 2004
Trade Name	NUZONE X2
Common Name	Sterile Neoprene - Polyisoprene Synthetic surgical glove, Powderfree, Polymer coated
Classification	Surgeon's Glove
Legally marketed device to which substantial equivalence is being claimed	The NUZONE X2, described in this 510(k) is substantially equivalent to the NUZONE Nitrile Surgical Gloves Powderfree that is currently marketed
Description of device	NUZONE X2 powderfree surgical glove meets the requirements for surgical gloves described by the American Standard for Testing and Material ASTM D 3577 - 01a <sup>2</sup>
Intended Use of the device	NUZONE X2 surgical gloves are disposable and sterile devices intended to be worn by healthcare personnel to prevent cross contamination between the user and the patient during procedures

510 K Summary ( continued)



## TERANG NUSA Sdn Bhd

510(k) Submission for NUZONE X2 Surgical Glove Powderfree

**Brief description of non-clinical tests**

Test conducted per ASTM D 3577 - 01a<sup>1</sup>, ASTM D512 indicates that the product meet the requirements.

Primary Skin Irritation test ASTM F 719-81 and Dermal Sensitization Test ASTM F 720-81 (86) indicates no sensitization or irritation

**Brief description of clinical tests**

Not required

**Conclusion drawn from clinical and non clinical tests**

It can be concluded that NUZONE X2 Neoprene - Polyisoprene synthetic powderfree surgical glove will perform according to the performance standards referenced and therefore meets ASTM standards, FDA requirements and labeling claims.

This device is substantially equivalent to the currently marketed devices.

**Additional information deemed necessary by the FDA**

None



AUG 20 2004

Mr. Chin-Guan Low  
Director  
Terang Nusa SDN BHD  
1, Jalan 8, Pengkalan  
Chepa 2 Industrial Zone,  
16100 Kota Bharu,  
MALAYSIA

Re: K041436

Trade/Device Name: Neoprene-Polyisoprene Synthetic Surgical Glove-Powderfree  
NUZONE X2

Regulation Number: 878.4460

Regulation Name: Surgeon's Glove

Regulatory Class: I

Product Code: KGO

Dated: August 6, 2004

Received: August 9, 2004

Dear Mr. Low:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.


If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please contact the Office of Compliance at (301) 594-4618. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address <http://www.fda.gov/cdrh/dsm/dsmmain.html>

Sincerely yours,



Chiu Lin, Ph.D.

Director

Division of Anesthesiology, General Hospital,

Infection Control and Dental Devices

Office of Device Evaluation

Center for Devices and

Radiological Health

Enclosure



## TERANG NUSA Sdn Bhd

510(k) Submission for NUZONE X2 Surgical Glove Powderfree

### 3. Indication for use Statement

Submitter	Terang Nusa Sdn Bhd
510(k) Number	K041436
Device Name	Neoprene - Polyisoprene Synthetic Surgical Glove - Powderfree
Trade Name	NUZONE X2

#### Indication for use

This surgical glove is a device made of a neoprene - polyisoprene synthetic material intended to be worn by operating room personnel to protect a surgical wound from contamination.

Prescription Use  Over the counter   
(Per 21 CFR 801 Subpart D) (21 CFR 807 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDHR Office of Device Evaluation (O.D.E.)

  
\_\_\_\_\_  
(Division Sign-Off)  
Division of Anesthesiology, General Hospital,  
Infection Control, Dental Devices  
510(k) Number K041436



**TOP GLOVE SDN. BHD.** (Company No. 220483-T)  
**TOP QUALITY, TOP EFFICIENCY,  
 GOOD HEALTH, SAFETY FIRST & BE HONEST**

\* A member of Top Glove Corporation Bhd, Public Listed Company on Bursa Malaysia.  
 Latex Examination, Nitrile, Surgical, Vinyl & Household Gloves Manufacturer and Exporter  
 The World's Largest Rubber Glove Manufacturer

Corporate Office : Lot 4969, Jalan Teratai, Batu 6, Off Jalan Meru, 41050 Klang, Selangor D. E., Malaysia.  
 & Factory 9 Tel: 603-3392 1992 / 1905 Fax: 603-3392 3410 / 1291  
 E-mail : sales@topglove.com.my Website : www.topglove.com.my



<b>BUSINESS DIRECTION</b>	: To Produce Consistently High Quality Gloves At Efficient Low Cost.
<b>FACILITIES</b>	: 27 Factories (Malaysia, Thailand & China), 486 Production Lines, 44 Billion Gloves Per Annum, 11,000 Employees
<b>MARKET</b>	: Exports to more than 195 countries worldwide with Marketing offices in the USA and Germany.

**DECLARATION OF CONFORMITY**


Manufacturer's Name : TOP GLOVE SDN. BHD  
 Manufacturer's Address : Lot 4969, Jalan Teratai, 6<sup>th</sup> Mile, Off Jalan Meru,  
 41050 Klang, Selangor D. E. Malaysia

Authorized Representative : NS LEGACY GROUP OF COMPANIES 5285959X  
 B3012 Mercu Summer Suite Jalan Cendana Off  
 Jalan Sultan Ismail 50250 Kuala Lumpur  
 Dato' Muhammad Syafiq Abdullah

Name of Device : Examination Gloves  
 Type : Powdered and Powder Free  
 Classification : Class I, Non Sterile  
 Conformity Assessment Procedure : Annex VII  
 Conformity Route : Self Declaration

We herewith declare with our own responsibility that above mentioned product(s) with CE mark is fully compliance with Essential Requirement of the EC Council Directive 93/42/EEC 14<sup>th</sup> June 1993 concerned medical devices, amended by Council Directive 2007/47/EC.

Registration Date : 31 March 2019  
 Registration No : DE/CA20/02-TOPGLOVEB-01/19  
 Date : 1<sup>st</sup> December 2019

  
 Name: Pn Noor Akilah Saidin  
 Designation: QA Deputy General Manager

RADOCIA



GERMANY



EUROPE



U.S.A.



AUSTRALIA



CANADA



MALAYSIA

**"To Prevent & Against Corruption" and "Be Honest, No Cheating"**

ASAL  
ORIGINAL

PIHAK BERKUASA  
PERANTI PERUBATAN



MEDICAL DEVICE  
AUTHORITY

**PIHAK BERKUASA PERANTI PERUBATAN**  
*MEDICAL DEVICE AUTHORITY*  
**AKTA PERANTI PERUBATAN 2012 (AKTA 737)**  
*MEDICAL DEVICE ACT 2012 (ACT 737)*  
**SIJIL PENDAFTARAN PERANTI PERUBATAN**  
*MEDICAL DEVICE REGISTRATION CERTIFICATE*  
**Seksyen 5(1) Akta 737**  
*Section 5(1) of Act 737*

No. Pendaftaran: **GMD26733243217A** Tarikh Sah Laku Pendaftaran: **25/08/2017 - 24/08/2022**  
*Registration No.:* *Registration Validity Date:*

Sijil ini adalah dengan ini dikeluarkan kepada:  
*This Certificate is hereby issued to:*

**TOP GLOVE SDN BHD**

yang beralamat di:  
*of:*

**LOT 4969, JALAN TERATAI, BATU 6,  
OFF JALAN MERU,  
KLANG  
41050 SELANGOR**

bagi mengesahkan peranti perubatan seperti yang dinyatakan dalam Lampiran 1 adalah berdaftar di bawah Seksyen 5(1) Akta 737.

*to confirm that the medical device as detailed out in Attachment 1 is registered under Section 5(1) of Act 737.*

Pendaftaran ini diberikan tertakluk kepada peruntukan-peruntukan di bawah Akta 737 dan peraturan-peraturan yang dibuat dibawahnya serta syarat-syarat seperti di Lampiran 2.

*This registration is granted subject to the provisions under Act 737 and its subsidiary legislations and the conditions as in Attachment 2.*



**ZAMANE BIN ABDUL RAHMAN**  
**Ketua Eksekutif**  
*Chief Executive*  
**Pihak Berkuasa Peranti Perubatan**  
*Medical Device Authority*

LAMPIRAN 1  
Attachment 1



No. Pendaftaran: **GMD26733243217A**  
Registration No.:

Butir-butir peranti perubatan yang didaftarkan  
Particulars of the registered medical device

Nama Peranti Perubatan Medical Device Name	<b>NITRILE EXAMINATION POWDER FREE GLOVES</b>		
Kelas Class	<b>CLASS A</b>	Brand Brand	<b>TOP GLOVE</b>
Kelompok Group	<b>FAMILY</b>		
Kegunaan Yang Diniatkan Intended Use	<b>TO WEAR ON HANDS OF HEALTHCARE PERSONNEL TO PREVENT CONTAMINATION BETWEEN HEALTHCARE PERSONNEL AND THE PATIENT.</b>		
Nama dan alamat pembuat: Name and address of manufacturer	<b>LOT 4969, JALAN TERATAI, BATU 6, OFF JALAN MERU, KLANG 41050 SELANGOR</b>		

**APPENDIX**

No.	NAME AS PER DEVICE LABEL	IDENTIFIER	BRIEF DESCRIPTION OF USE
1.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-S	SINGLE USE GLOVES
2.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-XS	SINGLE USE GLOVES
3.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-M	SINGLE USE GLOVES
4.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-L	SINGLE USE GLOVES
5.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-XL	SINGLE USE GLOVES
6.	NITRILE EXAMINATION POWDER FREE GLOVES	N02-XXL	SINGLE USE GLOVES



**TOP GLOVE SON BHD**  
**TEST REPORT**

Type Of Glove : **Nitrile Examination Chlorinated Powder Free Glove (Textured)**  
 Glove Code : **CW77**  
 AQL Required : **1.5**  
 Reference Standard : The above consignment of goods have been inspected against Top Glove standard where samples selected at random using Single Sampling Plans for Normal Inspection of ISO 2859-1.

Declared - Size :  
 - Quantity :

Size	Quantity (pcs)
S	100,000
M	100,000
L	100,000
Total	300,000

**1. Freedom from Holes and Visual Defects**

Size	Holes			Visual Defect (Inspection Level : G1)						Result
	Inspection level : G1, AQL 1.5			Major Defects, AQL 2.5			Minor Defects, AQL 4.0			
	Sample size (pcs)	Acceptance (pcs)	Defects (pcs)	Sample size (pcs)	Acceptance (pcs)	Defects (pcs)	Sample size (pcs)	Acceptance (pcs)	Defects (pcs)	
S	200	7	3	200	10	6	200	14	7	Pass
M	200	7	4	200	10	7	200	14	8	Pass
L	200	7	3	200	10	6	200	14	9	Pass

**2. Dimensions**

Inspection Level : S2, AQL 4.0  
 Acceptance : 1

Result : Pass

Sample No.	Size	Length (mm)	Width (mm)	Thickness (single wall) (mm)	
				Fingertip	Palm
1	S	300	84	0.17	0.16
2		299	85	0.17	0.15
3		301	85	0.14	0.13
4		302	86	0.15	0.14
5	M	298	97	0.16	0.14
6		299	96	0.14	0.15
7		300	95	0.17	0.16
8		301	96	0.15	0.13
9	L	297	106	0.16	0.14
10		303	105	0.16	0.14
11		301	106	0.16	0.15
12		299	104	0.14	0.15
13		302	105	0.15	0.14

ASTM D6319 – 10 (2015) Requirement:

Size	Length (mm)	Width (mm)	Thickness (mm)
XS	≥ 220	70 ± 10	Finger & Palm (Single wall) Min 0.05
S		80 ± 10	
M		95 ± 10	
L		110 ± 10	
XL		120 ± 10	

**3. Physical Properties**

Inspection Level : S2, AQL 4.0  
 Acceptance : 1

Result : Pass

Sample No.	Size	Before Aging		After Accelerated Aging	
		Tensile Strength (MPa)	Elongation %	Tensile Strength (MPa)	Elongation %
1	S	19.2	573	15.4	452
2		15.4	567	16.1	458
3		17.5	532	15.6	532
4		17.1	602	16.0	472
5	M	16.7	554	16.5	498
6		17.3	601	17.1	505
7		18.4	546	18.1	470
8		18.3	587	16.2	481
9	L	18.3	612	16.3	484
10		16.7	598	15.8	538
11		17.4	576	16.2	486
12		18.9	563	17.1	514
13		15.9	591	16.3	474

ASTM D6319 – 10 (2015) Requirement:

Before Aging		After Accelerated Aging	
Tensile	Elongation	Tensile	Elongation
Min 14 MPa	Min 500%	Min 14 MPa	Min 400%

Note:

A test result is the median of three individual test measurement values.

**4. Powder Residue**

Sampling size, N = 5  
 Requirement: Max 2 mg / glove

Size	mg / glove	Result
S	0.8	Pass
M	1.2	Pass
L	0.6	Pass

**CONCLUSION :** We hereby certify that the above consignment of goods were determined to meet the acceptable limit of the specifications as referring to the above findings of randomly selected samples.

Prepared By : Dayana Azman  
 QA Chemist II

Verified By : Noor Akilah Saadin  
 QA Deputy General Manager



October 12, 2019

Top Glove SDN BHD  
Noor Akilah Bt Saidin  
Deputy General Manager, QA  
Lot 4968, Jalan Teratai, Batu 6, Off Jalan Meru  
Klang, 41050 MY

Re: K191279

Trade/Device Name: Sterile Latex Surgical Powder Free Gloves; Sterile Nitrile Surgical Powder Free Gloves Tested for Use with Chemotherapy Drugs

Regulation Number: 21 CFR 880.6250

Regulation Name: Surgeon's Gloves

Regulatory Class: Class I

Product Code: KGO, LZA, LZC

Dated: September 13, 2019

Received: September 13, 2019

Dear Noor Akilah Bt Saidin:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you, however, that device labeling must be truthful and not misleading.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the [Federal Register](#).

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR

Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please contact the Division of Industry and Consumer Education (DICE) at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address

<http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to

<http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

You may obtain other general information on your responsibilities under the Act from the Division of Industry and Consumer Education (DICE) at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address

<http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>.

Sincerely,

**Michael J. Ryan -S**

for Tina Kiang, PhD  
Acting Director  
Division of Anesthesiology,  
General Hospital, Respiratory,  
Infection Control, and Dental Devices  
Office of Device Evaluation  
Center for Devices and Radiological Health

Enclosure

### Indications for Use

510(k) Number (if known)

K191279

Device Name

Sterile Nitrile Surgical Powder Free Gloves Tested for Use with Chemotherapy Drugs

Indications for Use (Describe)

Sterile Nitrile Surgical Powder Free Gloves Tested for Use with Chemotherapy Drugs is to be worn on the hands of healthcare professionals during surgery to prevent cross contamination between healthcare personnel and the patient.

These gloves are tested for use with Chemotherapy Drugs as per ASTM D6978-05 Standard Practice for Assessment of Medical Gloves to Permeation by Chemotherapy Drugs.

Chemotherapy Drug Permeation

The following chemicals have been tested with these gloves.

Chemotherapy Drug	Concentration	Breakthrough Detection Time in Minutes
Carmustin (BCNU)	3.3mg/ml	8.0
Cisplatin	1.0mg/ml	>240
Cyclophosphamide (Cytosan)	20.0mg/ml	>240
Dacarbazine (DTIC)	10.0mg/ml	>240
Doxorubicin Hydrochloride	2.0mg/ml	>240
Etoposide (Toposar)	20.0mg/ml	>240
Fluorouracil	50.0mg/ml	>240
Paclitaxel (Taxol)	6.0mg/ml	>240
Thiotepa	10.0mg/ml	16.2

\* Please note that the following drugs have extremely low permeation times:

Carmustin (BCNU) : 8.0 minutes and Thiotepa : 16.2 minutes

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D)

Over-The-Counter Use (21 CFR 801 Subpart C)

#### CONTINUE ON A SEPARATE PAGE IF NEEDED.

This section applies only to requirements of the Paperwork Reduction Act of 1995.

**\*DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW.\***

The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services  
Food and Drug Administration  
Office of Chief Information Officer  
Paperwork Reduction Act (PRA) Staff  
PRASStaff@fda.hhs.gov

*\*An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number.\**

### Indications for Use

510(k) Number (if known)

K191279

Device Name

Sterile Latex Surgical Powder Free Gloves

Indications for Use (Describe)

Sterile Latex Surgical Powder Free Gloves is to be worn on the hands of healthcare professionals during surgery to prevent cross contamination between healthcare personnel and the patient.

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D)

Over-The-Counter Use (21 CFR 801 Subpart C)

#### CONTINUE ON A SEPARATE PAGE IF NEEDED.

This section applies only to requirements of the Paperwork Reduction Act of 1995.

**\*DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW.\***

The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services  
Food and Drug Administration  
Office of Chief Information Officer  
Paperwork Reduction Act (PRA) Staff  
PRAStaff@fda.hhs.gov

*"An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number."*



**FDA** U.S. FOOD & DRUG  
ADMINISTRATION

April 26, 2018

Top Glove SDN. BHD.  
Noor Saidin  
QA Deputy General Manager  
Lot 4968, Jalan Teratai,  
Batu 6, Off Jalan Meru  
41050 Klang, Selangor  
Malaysia

Re: K172923

Trade/Device Name: Nitrile Examination Powder Free Glove, White, Black, Orange  
Nitrile Examination Powder Free Gloves Tested For Use With Chemotherapy  
Drugs, Blue

Regulation Number: 21 CFR 880.6250

Regulation Name: Patient Examination Glove

Regulatory Class: I

Product Code: LZA, LZC

Dated: March 27, 2018

Received: April 9, 2018

Dear Noor Saidin:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you, however, that device labeling must be truthful and not misleading.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the [Federal Register](#).

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

For comprehensive regulatory information about medical devices and radiation-emitting products, including information about labeling regulations, please see Device Advice (<https://www.fda.gov/MedicalDevices/DeviceRegulationandGuidance/>) and CDRH Learn (<http://www.fda.gov/Training/CDRHLearn>). Additionally, you may contact the Division of Industry and Consumer Education (DICE) to ask a question about a specific regulatory topic. See the DICE website (<http://www.fda.gov/DICE>) for more information or contact DICE by email ([DICE@fda.hhs.gov](mailto:DICE@fda.hhs.gov)) or phone (1-800-638-2041 or 301-796-7100).

Sincerely,

**Geeta K.  
Pamidimukkala -S**

for Tina Kiang, Ph.D.  
Acting Director  
Division of Anesthesiology,  
General Hospital, Respiratory,  
Infection Control, and Dental Devices  
Office of Device Evaluation  
Center for Devices and Radiological Health

Enclosure

### Indications for Use

510(k) Number (if known)

K172923

Device Name

Nitrile Examination Powder Free Glove, White

Indications for Use (Describe)

A patient examination glove is a disposable device intended for medical purpose that is worn on the examiner's hand or finger to prevent contamination between patient and examiner.

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D)

Over-The-Counter Use (21 CFR 801 Subpart C)

**CONTINUE ON A SEPARATE PAGE IF NEEDED.**

This section applies only to requirements of the Paperwork Reduction Act of 1995.

**\*DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW.\***

The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services  
Food and Drug Administration  
Office of Chief Information Officer  
Paperwork Reduction Act (PRA) Staff  
PRASStaff@fda.hhs.gov

*\*An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number.\**

## Indications for Use

510(k) Number (if known)  
K172923

Device Name  
Nitrile Examination Powder Free Glove, Orange

Indications for Use (Describe)

A patient examination glove is a disposable device intended for medical purpose that is worn on the examiner's hand or finger to prevent contamination between patient and examiner.

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D)  Over-The-Counter Use (21 CFR 801 Subpart C)

### CONTINUE ON A SEPARATE PAGE IF NEEDED.

This section applies only to requirements of the Paperwork Reduction Act of 1995.

**\*DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW.\***

The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services  
Food and Drug Administration  
Office of Chief Information Officer  
Paperwork Reduction Act (PRA) Staff  
[PRASStaff@fda.hhs.gov](mailto:PRASStaff@fda.hhs.gov)

*\*An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number.\**

## Indications for Use

510(k) Number (if known)  
K172923

Device Name

Nitrile Examination Powder Free Glove Tested for Use with Chemotherapy Drugs, Blue

Indications for Use (Describe)

A patient examination glove is a disposable device intended for medical purpose that is worn on the examiner's hand or finger to prevent contamination between patient and examiner.

These gloves were tested for use with Chemotherapy Drugs as per ASTM D6978-05 standard practice for assessment of medical gloves to permeation by chemotherapy drugs:

Chemotherapy Drug Permeation

The following chemicals have been tested with these gloves.

Chemotherapy Drugs	Concentration	Breakthrough Detection Time in Minutes
Carmustine (BCNU)	3.3 mg/ml	15.9
Ciplastin	1.0 mg/ml	> 240
Cyclophosphamide (Cytosan)	20.0 mg/ml	> 240
Dacarbazine (DTIC)	10.0 mg/ml	> 240
Doxorubicin Hydrochloride	2.0 mg/ml	> 240
Etoposide (Toposar)	20.0 mg/ml	> 240
Fluorouracil	50.0 mg/ml	> 240
Paclitaxel (Taxol)	6.0 mg/ml	> 240
Thiotepa	10.0 mg/ml	47.3

Please note that the following drugs have low permeation time :  
Carmustine (BCNU): 15.9 minutes and Thiotepa: 47.3 minutes

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D)  Over-The-Counter Use (21 CFR 801 Subpart C)

### CONTINUE ON A SEPARATE PAGE IF NEEDED.

This section applies only to requirements of the Paperwork Reduction Act of 1995.

**\*DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW.\***

The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services  
Food and Drug Administration  
Office of Chief Information Officer  
Paperwork Reduction Act (PRA) Staff  
PRAStaff@fdh.hhs.gov

*"An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number."*







AWARDED  
ISO 9001

**TOP GLOVE SDN. BHD.** (Company No. 220483-T)

**TOP QUALITY, TOP EFFICIENCY,  
GOOD HEALTH, SAFETY FIRST & BE HONEST**

\* A member of Top Glove Corporation Bhd, Public Listed Company on Bursa Malaysia.  
Latex Examination, Nitrile, Surgical, Vinyl & Household Gloves Manufacturer and Exporter  
The World's Largest Rubber Glove Manufacturer

Corporate Office : Lot 4969, Jalan Teratai, Batu 6, Off Jalan Meru, 41050 Klang, Selangor D. E., Malaysia.  
& Factory 9 Tel: 603-3392 1992 / 1905 Fax: 603-3392 8410 / 1291  
E-mail : sales@topglove.com.my Website : www.topglove.com.my



<b>BUSINESS DIRECTION</b>	: To Produce Consistently High Quality Gloves At Efficient Low Cost.
<b>FACILITIES</b>	: 27 Factories (Malaysia, Thailand & China), 485 Production Lines, 44 Billion Gloves Per Annum, 11,000 Employees
<b>MARKET</b>	: Exports to more than 195 countries worldwide with Marketing offices in the USA and Germany.

## EC DECLARATION OF CONFORMITY

Manufacturer's Name : TOP GLOVE SDN. BHD  
 Manufacturer's Address : Lot 4969, Jalan Teratai, 6<sup>th</sup> Mile, Off Jalan Meru,  
 41050 Klang, Selangor D. E. Malaysia

European Authorized Representative : Top Glove Europe GmbH  
 Bliersheimer Str. 80, D-47229 Duisburg  
 Deutschland/Germany  
 Tel.:+49-(0)2065-76421-0, Fax:+49-(0)2065-76421-19


Name of Device : Nitrile Examination Gloves  
 Type : Powdered and Powder Free  
 Classification : Class I, Non Sterile  
 Conformity Assessment Procedure : Annex VII  
 Conformity Route : Self Declaration

We herewith declare with our own responsibility that above mentioned product(s) with CE mark is fully compliance with Essential Requirement of the EC Council Directive 93/42/EEC 14<sup>th</sup> June 1993 concerned medical devices, amended by Council Directive 2007/47/EC.

Competent Authority : Bezirksregierung Düsseldorf,  
 Postfach 300865, 40408 Düsseldorf.

Registration Date : 31 March 2010  
 Registration No : DE/CA20/02-TOPGLOVEB-01/10

Date : 1<sup>st</sup> December 2016

  
 Name: Pn Noor Akilah Saidin  
 Designation: QA Deputy General Manager

RADOC/A



GERMANY



EUROPE



U.S.A.



AUSTRALIA



CANADA



MALAYSIA

**"To Prevent & Against Corruption" and "Be Honest, No Cheating"**

November 22, 2019

• **TEST REPORT** •

PN 127526

**CHEMICAL ANALYTICAL SERVICES**


Prepared For:

Noor Hazwa Hashim  
**Top Glove Sdn. Bhd.**  
Lot 4969, Jalan Teratai,  
Batu 6, Off Jalan Meru  
41050 Klang, Selangor D.E.  
Malaysia

Prepared By:

  
Tiffany L. Heller  
Assistant Manager  
Pharmaceutical Services

Approved By:

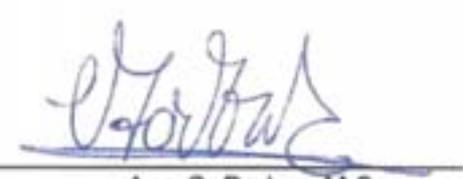  
Ana C. Barbur, M.S.  
Manager  
Chemical, Microbiological, & Pharmaceutical Services



An A2LA Accredited Testing Laboratory — Certificate Numbers 255.01 & 255.02  
ISO 9001:2008 Registered

**ISO 9001:2008**  
Registered

Letters and reports are for the exclusive use of the clients to whom they are addressed and shall not be reproduced, except in full, without the written permission of Akron Rubber Development Laboratory, Inc. (ARDL). The information contained herein applies to the specific material, products or processes tested or evaluated. No warranty of any kind is herein construed or implied. The liability of ARDL, Inc. shall be limited to the amount of consideration paid for services. ARDL, Inc. is accredited by A2LA for the test methods listed on the attached scope.

November 22, 2019

Noor Hazma Hashim  
Top Glove Sdn. Bhd.

Page 1 of 2 – PN 127526

**SUBJECT:** Permeation testing per ASTM D 6978-05 on sample submitted by the above company.

**RECEIVED:** One bag of blue gloves identified as Nitrile Examination Powder Free Glove, CW77.

**TESTING CHEMOTHERAPY DRUGS:**

Table 1. List of the Testing Chemotherapy Drugs, Sources, and Expiration Dates

TESTING CHEMOTHERAPY DRUGS	DRUG SOURCE
Carmustine (BCNU)	Sigma Aldrich; Lot# 015M4004V; Expiration 04/2016
Thiotepa	Sigma Aldrich; Lot# SLBM7142V; Expiration 02/2016

**COLLECTION MEDIA:**

The collection media which were selected are listed in Table 2.

Table 2. Collection Media for Testing Chemotherapy Drugs

TEST CHEMICAL AND CONCENTRATION	COLLECTION MEDIUM
Carmustine (BCNU), 3.3 mg/ml (3,300 ppm)	10% Ethanol Aqueous Solution
Thiotepa, 10.0 mg/ml (10,000 ppm)	Distilled Water

**TESTING CONDITIONS:**

Standard Test Method Used:	ASTM D 6978-05
Analytical Method:	UV/VIS Spectrometry
Testing Temperature:	35.0°C ± 2.0
Collection System:	Closed Loop
Specimen Area Exposed:	5.067 cm <sup>2</sup>
Selected Data Points:	25/test
Number of Specimens Tested:	3/test
Location Sampled From:	Cuff area

**DETECTION METHOD OF CHEMICAL PERMEATION; UV/VIS ABSORPTION SPECTROMETRY:**

Instrument: Perkin Elmer UV/VIS Spectrometer Lambda 25

UV/VIS Absorption Spectrometry was used to measure the absorbance of test chemicals which permeated through the specimens into the collection medium. The collection medium was circulated in a closed loop at 11 ml/minute of flow rate through the testing period. Data collection was performed according to the programmed schedule by means of UV Winlab software from the Perkin Elmer Corporation. The list of the characteristic wavelengths is shown below.

Table 3. Characteristic Wavelengths used in UV/VIS Absorption Spectrometry

TESTING CHEMOTHERAPY DRUGS	WAVELENGTH (nm)
Carmustine (BCNU)	229
Thiotepa	199

**SAMPLE CHARACTERISTICS:**


Table 4. Thickness characteristics for the tested specimens on: Nitrile Examination Powder Free Glove, CW77.

Testing Chemotherapy Drugs	Thickness (mm)			Average (mm)	Weight/Unit Area (g/m <sup>2</sup> )
	#1	#2	#3		
Carmustine (BCNU)	0.098	0.099	0.096	0.098	100.4
Thiotepa	0.099	0.103	0.093	0.098	


**RESULTS:**

Table 5. Permeation Test Results on: Nitrile Examination Powder Free Glove, CW77.

TEST CHEMOTHERAPY DRUG AND CONCENTRATION	MINIMUM BREAKTHROUGH DETECTION TIME (Specimen1/2/3) (Minutes)	AVERAGE STEADY STATE PERM. RATE (Specimen1/2/3) (µg/cm <sup>2</sup> /minute)	OTHER OBSERVATIONS
Carmustine (BCNU), 3.3 mg/ml (3,300 ppm)	50.3 (50.3,52.8,53.2)	0.6 (0.6,0.6,0.7)	Moderate swelling and slight degradation
Thiotepa, 10.0 mg/ml (10,000 ppm)	150.6 (150.6,160.4,160.5)	0.2 (0.2,0.2,0.2)	Slight swelling and no degradation

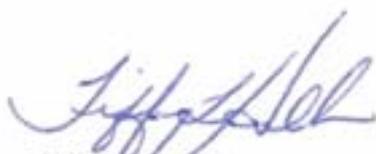

Tiffany L. Heller  
Assistant Manager  
Pharmaceutical Services

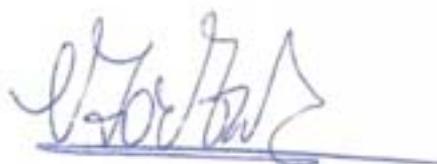

Ana C. Barbur, M.S.  
Manager  
Chemical, Microbiological and Pharmaceutical Services

## TOP GLOVE SDN. BHD.

**PRODUCT SPECIFICATION**  
**Nitrile Powder Free Examination Gloves (Palm Textured)**

**SECTION I: PRODUCT DESCRIPTION**

1.1	Type	Nitrile Examination Glove, Powder Free, Online Single Chlorinated, Non-sterile
1.2	Material	100% Synthetic Nitrile Latex
1.3	Color	Blue
1.4	Design and Feature	Ambidextrous, palm textured, beaded cuff
1.5	Powder	No powder lubricant added
1.6	Storage Condition	The gloves shall maintain their properties when stored in a dry condition. Avoid direct sunlight.
1.7	Shelf-Life	The gloves shall have shelf life of 5 years from the date of manufacture with the above storage condition.
1.8	Packing Style	100 pcs gloves x 10 dispensers x 1 carton
1.9	Size Marking	The size of gloves shall be marked in the check box on every carton with black ink.

**SECTION II: PERFORMANCE REQUIREMENTS**

(Sampling Plan – ISO 2859 Single Normal)

#	Characteristics	Inspection Level	Acceptable Quality Level	Reference Standard
2.1	Dimensions	S2	4.0	ASTM D6319-10 (2015)
2.2	Physical Properties	S2	4.0	ASTM D6319-10 (2015)
2.3	Freedom from Holes (Air Pump Test)	G1	1.5	In-house practice
2.4	Visual Defects:			
(i)	Major Visual	G1	2.5	In-house practice
(ii)	Minor Visual		4.0	
2.5	Packaging Defects:			
(i)	Regulatory	G1	**	In-house practice
(ii)	Visual	G1	4.0	
(iii)	Critical (incl. Gloves Counting)	S2	4.0	
2.6	Powder Free Residue	N=5	-	ASTM D6319-10 (2015) ASTM D6124-06 (2011)
2.7	Mix Size / Mix Glove / Mix Hand	Not Allowed		

\*\*Unacceptable at any level

## TOP GLOVE SDN. BHD.

## SECTION III: PERFORMANCE SPECIFICATION

## 3.1 Dimensions

Description	Size	Standard
Length (mm)	All Sizes	300 +/- 10
Palm Width (mm)	XS	76 +/- 3
	S	84 +/- 3
	M	94 +/- 3
	L	105 +/- 3
	XL	113 +/- 3
	XXL	123 +/- 3
Thickness (mm) *single wall	All Sizes	Finger : 0.15 +/- 0.02 (Typical value: 0.14 – 0.17)  Palm : 0.14 +/- 0.02 (Typical value: 0.13 – 0.16)

## 3.2 Physical Properties

Description	Standard	
	Before Aging	After Aging
Elongation at Break (%)	Min 500 (Typical value: 500 - 600)	Min 400 (Typical value: 400 - 550)
Tensile Strength (MPa)	Min 14 (Typical value: 14 - 20)	Min 14 (Typical value: 14 - 20)

## 3.3 Freedom from Holes

The sample size and allowable number of non-conforming gloves in the samples shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements.

## 3.4 Visual Defects

The sample size and allowable number of non-conforming gloves in the samples for both major and minor defects shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements.

## 3.5 Packaging Defects

The Sample size and allowable number of non-conforming in the samples for regulatory, visual and critical packaging defects shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements (Gloves Counting=100 pcs by weight per Dispenser).

## 3.6 Powder Free Residue

Maximum 2 mg per glove

Prepared by:  
Quality Product Management System Division

Date: 17<sup>th</sup> May 2017

Checked by:  
Eva Vinoni Bt Mustafa  
Senior Manager, QA

Approved by:  
Noor Akilah Saidin  
Deputy General Manager, QA

**TOP GLOVE SDN. BHD.**

**PRODUCT SPECIFICATION**  
**Nitrile Powder Free Examination Gloves (Palm Textured)**

---

**SECTION I: PRODUCT DESCRIPTION**

1.1	Type	Nitrile Examination Glove, Powder Free, Online Single Chlorinated, Non-sterile
1.2	Material	100% Synthetic Nitrile Latex
1.3	Color	Blue
1.4	Design and Feature	Ambidextrous, palm textured, beaded cuff
1.5	Powder	No powder lubricant added
1.6	Storage Condition	The gloves shall maintain their properties when stored in a dry condition. Avoid direct sunlight.
1.7	Shelf-Life	The gloves shall have shelf life of 5 years from the date of manufacture with the above storage condition.
1.8	Packing Style	100 pcs gloves x 10 dispensers x 1 carton
1.9	Size Marking	The size of gloves shall be marked in the check box on every carton with black ink.

**SECTION II: PERFORMANCE REQUIREMENTS**

(Sampling Plan – ISO 2859 Single Normal)

#	Characteristics	Inspection Level	Acceptable Quality Level	Reference Standard
2.1	Dimensions	S2	4.0	ASTM D6319-10 (2015)
2.2	Physical Properties	S2	4.0	ASTM D6319-10 (2015)
2.3	Freedom from Holes (Air Pump Test)	GI	1.5	In-house practice
2.4	Visual Defects:			
(i)	Major Visual	GI	2.5	In-house practice
(ii)	Minor Visual		4.0	
2.5	Packaging Defects:			
(i)	Regulatory	GI	**	In-house practice
(ii)	Visual	GI	4.0	
(iii)	Critical (incl. Gloves Counting)	S2	4.0	
2.6	Powder Free Residue	N=5	-	ASTM D6319-10 (2015) ASTM D6124-06 (2011)
2.7	Mix Size / Mix Glove / Mix Hand	Not Allowed		

\*\*Unacceptable at any level

**TOP GLOVE SDN. BHD.****SECTION III: PERFORMANCE SPECIFICATION**

## 3.1 Dimensions

Description	Size	Standard
Length (mm)	All Sizes	300 +/- 10
Palm Width (mm)	XS	76 +/- 3
	S	84 +/- 3
	M	94 +/- 3
	L	105 +/- 3
	XL	113 +/- 3
	XXL	123 +/- 3
Thickness (mm) *single wall	All Sizes	Finger : 0.15 +/- 0.02 (Typical value: 0.14 – 0.17)  Palm : 0.14 +/- 0.02 (Typical value: 0.13 – 0.16)

## 3.2 Physical Properties

Description	Standard	
	Before Aging	After Aging
Elongation at Break (%)	Min 500 (Typical value: 500 - 600)	Min 400 (Typical value: 400 - 550)
Tensile Strength (MPa)	Min 14 (Typical value: 14 - 20)	Min 14 (Typical value: 14 - 20)

## 3.3 Freedom from Holes

The sample size and allowable number of non-conforming gloves in the samples shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements.

## 3.4 Visual Defects

The sample size and allowable number of non-conforming gloves in the samples for both major and minor defects shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements.

## 3.5 Packaging Defects

The Sample size and allowable number of non-conforming in the samples for regulatory, visual and critical packaging defects shall be determined in accordance to Sampling Plan ISO 2859-1 Single Normal using inspection and acceptable quality level as stated in Section II: Performance Requirements (Gloves Counting=100 pcs by weight per Dispenser).

## 3.6 Powder Free Residue

Maximum 2 mg per glove

Prepared by:  
Quality Product Management System Division

Date: 17<sup>th</sup> May 2017

Checked by:  
Eva Vinoni Bt Mustafa  
Senior Manager, QA

Approved by:  
Noor Akilah Saidin  
Deputy General Manager, QA